


AI4CMR Software

User Manual

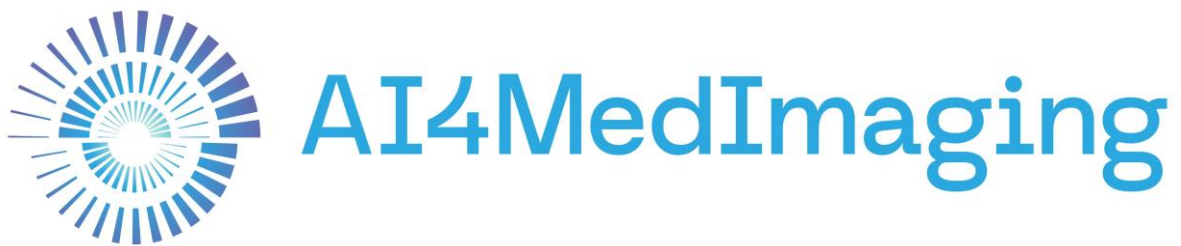

July 1, 2024

SW Version V1.4



Manufactured by

AI4MedImaging Medical Solutions S.A.

SRN PT-MF-000002951

Address

Rua do Parque Poente, Lote 35
4705-002 Sequeira, Braga
Portugal

Email

support@ai4medimaging.com

Website

<https://ai4medimaging.com/>

UK Responsible Person

UKCApartner4U Limited

Address

Campion Way, Bingham,
Nottingham NG13 8TR,
United Kingdom

Email

office@cepartner4u.com

Website

<https://www.cepartner4u.com/>



AI4CMR is qualified as a class IIa medical device.
It complies with the requirements of the European
Medical Device Regulation MDR 2017/745

MDR Certificate MDR 740464

UDI-DI (01)05600250059015



Swiss Authorised Representative

Alpha Innomed Sàrl.

CHRN-AR-20001545

Address

Saint Laurent, 17A
1176 Saint-Livres
Schweiz

Email

joaquin.azpilicueta@alpha-innomed.com



Swiss Importer

Alpha Innomed Sàrl.

Address

Saint Laurent, 17A
1176 Saint-Livres
Schweiz

Email

joaquin.azpilicueta@alpha-innomed.com



ISO 13485:2016 Certificate
MD 740465



AI4CMR is qualified as a class IIa medical device.
It complies with the requirements of the Medical
Device Directive 93/42/EEC and UK MDR 2002.

UKCA Certificate UKCA 776320

This user's manual is protected by copyright unless exclusively authorized in writing, its dissemination, duplication, or other commercial exploitation of this documentation or communication of its contents or parts of it is not permitted.

AI4MedImaging shall not be responsible for technical or editorial errors or omissions contained herein.

The information contained herein is subject to change without notice.

The only warranties for AI4MedImaging products and services are described in the express warranty statements accompanying such products and services.

Please contact the manufacturer or authorized representative to request the latest edition of the user manual or consult the latest edition on the AI4MedImaging website.

Table of Contents

Table of Contents	4
1. Terms and Conditions	5
1.1 Intended use	5
1.2 Intended users	5
1.3 Conditions for use	6
1.4 Contraindications	7
1.5 Limitations	7
1.6 Warnings and precautions	7
1.7 Intended patient population	8
1.8 Applicable medical conditions	8
1.9 Safety Instructions	8
2. Conventions and Abbreviations	9
2.1 Conventions	9
2.2 Abbreviations	9
3. Getting Started	10
3.1 Notice to the user	10
3.2 System requirements	10
3.3 Setup	10
3.4 User Training	11
3.5 Software overview	12
3.5.1 General operating steps	13
3.5.2 Summary of outputs validation	15
3.5.3 Plugin	16
4. User account handling	23
4.1 Authentication	23
4.2 User information handling	23
4.3 Password handling	24
4.4 Open sessions	24
4.5 Logging info	25
5. Technical Support	26

1. Terms and Conditions

This User Manual shall be accompanied by the specific plugin User Manual. The plugin User Manual describes in more detail the features and steps necessary to interact with the AI4CMR service. For clarification purposes only, we present an example of a possible sequence of steps to interact with AI4CMR.

1.1 Intended use

AI4CMR is an image analysis software for post-processing of cardiac magnetic resonance images (CMR), which are used for the assessment of cardiac diseases.

AI4CMR uses artificial intelligence and is intended to automatize cardiac segmentation allowing instantaneous quantification of ventricular volumes, myocardial mass, ejection fraction of heart ventricles and to automatically assess left ventricle wall motion.

AI4CMR shall be used by qualified medical professionals, experienced in examining and evaluating magnetic resonance images as a support tool that provides relevant clinical information.

AI4CMR can be integrated with DICOM viewers through a standard communication protocol.

The software is not intended to determine or recommend a course of action or treatment for a patient.

AI4CMR software does not preclude the analysis of the reporting physician. The cine sequences analysed by AI4CMR are only a part of the complete CMR exam and all the data should be integrated with other sequences and the clinical background of the patient to conclude the CMR exam.

The reporting physician holds the responsibility for validating the data provided by the AI4CMR software and performing the final interpretation of the CMR exam.

1.2 Intended users

AI4CMR is a medical device and shall be used by qualified medical professionals, experienced in examining and evaluating magnetic resonance images.

1.3 Conditions for use

AI4CMR is a cloud-hosted service. The system shall be used in association with a third-party DICOM Viewer, which provides the interface between AI4CMR and the intended users (Medical professionals), Software Developers, and Others.

Patients will not be in direct contact with AI4CMR. The CMR images acquired for the patient are fed from the MRI Scanner or PACS (picture archiving and communication system) to the third-party DICOM Viewer.

This system context and interfaces to third-party systems are represented in the diagram of Figure 1. The AI4CMR system boundaries, are defined by the box “AI4CMR”.

The integration between AI4CMR and the DICOM Viewer is established using plugins that implement a standard communication protocol.

The communication between AI4CMR and the third-party system is initiated by the third-party system which posts a request to the AI4CMR in a networked environment. AI4CMR will validate and process the request and return a response via the same medium.

The patient data is anonymized by the third party before being sent to AI4CMR.

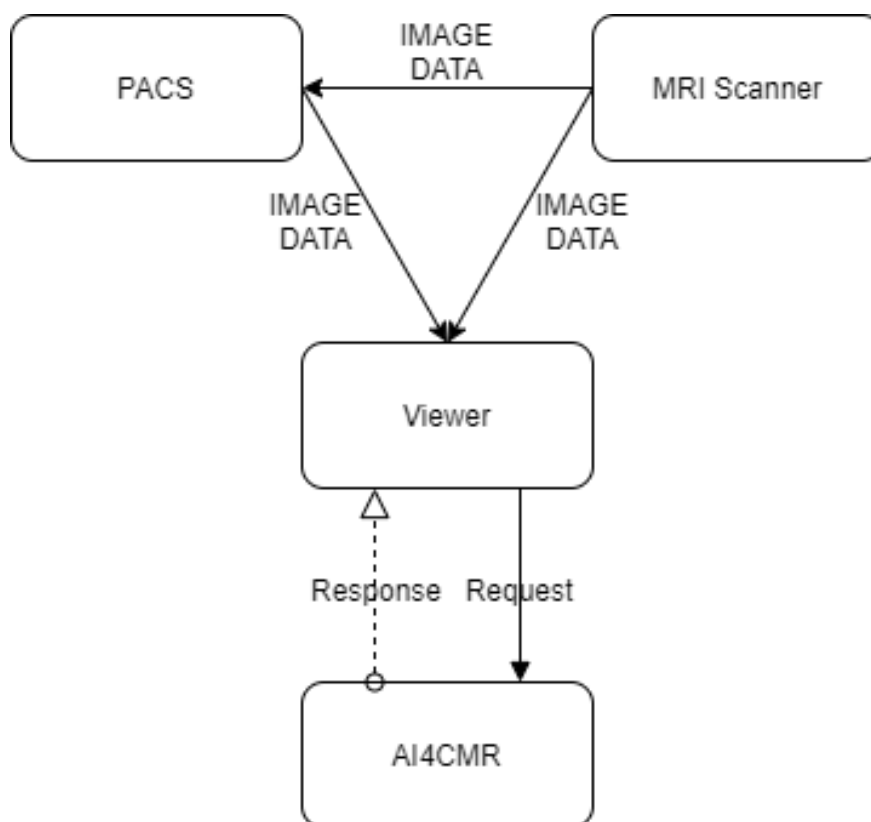


Figure 1. High-level representation of the interoperability between AI4CMR and the third-party systems and services.

1.4 Contraindications

AI4CMR is contraindicated to be used for post-processing of all image modalities other than cine CMR.

1.5 Limitations

AI4CMR analysis is limited to cine CMR acquisitions.

Other studies such as Late Gadolinium Enhancement or Perfusion are not covered.

AI4CMR's performance has been tested in three MRI scanner vendors: Siemens, GE Healthcare Systems and Phillips Medical Systems. For new MRI scanner vendors, a message will be returned to the User stating that the vendor is not valid.

AI4CMR's performance has been validated for a range of image characteristics. Cases with image characteristics that are outside the boundaries of the verified performance of the algorithms will be rejected.

1.6 Warnings and precautions

- The physician must always review the cases even when AI4CMR classifies them as normal.
- Quantitative analysis is dependent on the quality and correctness of the image source data acquisition.
- The patient data must be anonymized by the third-party plugin before sending it to AI4CMR.
- The patient data displayed is initially derived from the DICOM information, if available. Editing these values may affect the calculations in all modules. It is the User's responsibility to verify this data before releasing the final results.
- The User must keep a UPS system that provides emergency power when the input power source or mains power fails.
- It is the plugin maintenance team's responsibility to execute the installation procedure to validate the communication between the User and AI4CMR.
- It is AI4MedImaging's responsibility to update/do maintenance periodically to reduce the probability of AI4CMR SW defects.
- At the installation time, a copy of the digital user manual must be copied to the User's network, under the domain of the User's IT Manager.
- In the event of loss of access credentials please follow the procedure in section 4. User account handling.
- Users should read this manual before using AI4CMR.

1.7 Intended patient population

The software analyses images of patients that were examined by CMR imaging.

Age The use is not recommended for children (age < 18yo) since the clinical evaluation studies targeted a mostly adult population.

Weight No limitations

Height No limitations

1.8 Applicable medical conditions

AI4CMR is an image analysis software for the post-processing of CMR images, used for the assessment of the following cardiac diseases:

- Cardiac failure
- Ischemic heart disease
- Valvular heart disease
- Cardiomyopathy
- Cardiac function and morphology
- Hypertensive cardiac disease
- Other pathologies that need assessment of cardiac function and morphology

1.9 Safety Instructions

Software AI4CMR is hosted in a cloud. The intended users interact remotely with the software.

The equipment communicating with AI4CMR shall:

- Be connected to a secure network;
- Have an access control system, to ensure that only accredited users can access the device and the AI4CMR service.

AI4CMR requires that the passwords are different from the username and have at least:

- Eight (8) characters;
- One (1) digit;
- One (1) uppercase;
- One (1) lowercase;
- One (1) special character.

It is highly recommended the usage of anti-virus software in all computers interacting with the AI4CMR to protect against cyber-attacks. Periodic backups are also recommended to make sure that no patient data is lost in an unforeseen event.

2. Conventions and Abbreviations

2.1 Conventions

EDV – End-Diastolic Volume [ml]

ESV – End-Systolic Volume [ml]

SV – Stroke Volume [ml]

EF – Ejection Fraction [%]

Mass – Myocardial Mass [g]

CO – Cardiac Output [L/min]

EDV/BSA – End-Diastole Volume/Body Surface Area [ml/m²]

ESV/BSA - End-Systole Volume/Body Surface Area [ml/m²]

SV/BSA – Systole Volume/Body Surface Area [ml/m²]

Mass/BSA – Myocardial Mass/Body Surface Area [g/m²]

CI – Cardiac Index [L/(min m²)]

BSA - Body Surface Area [m²]

2.2 Abbreviations

ED – End-Diastole

ES – End-Systole

MRI – Magnetic Resonance Imaging

CMR – Cardiac Magnetic Resonance

DICOM – Digital Imaging and Communications in Medicine

HTTP – Hypertext Transfer Protocol

SA – Short-axis

LA – Long-axis

LV – Left Ventricle

RV – Right Ventricle

ICC - Interclass Correlation Coefficient

3. Getting Started

3.1 Notice to the user

Any serious incident that has occurred in relation to the device should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.

3.2 System requirements

AI4CMR software runs as a Docker image on the cloud.
The minimum requirements for the ethernet connection are:

- High bandwidth network (50Mbps/s minimum and 100Mbps/s recommended).

3.3 Setup

For customer registration, the customer environment shall be informed to AI4MedImaging: MRI scanner vendor, PACS vendor and version, Viewer vendor and version and third-party plugin ID and version.

A *client_id* and temporary user authentication credentials will be assigned by AI4MedImaging to the customer.

The third-party plugin shall be installed and configured as per its User Manual.

To validate the set-up, the following validation protocol shall be followed:

1. Three clinical cases (hereinafter called gold samples GS1; GS2 and GS3) are delivered to the customer by AI4MedImaging. The samples shall be submitted to AI4CMR through the third-party plugin.

GS1 case is a valid case with all the mandatory and optional data;
GS2 case is a valid case with all the mandatory data;
GS3 case is a non-valid case with missing mandatory data.

2. The results displayed by the third-party plugin for each of the golden samples shall be compared with the following expected results:

GS1:

	EDV (mL)	IEDV index (mL/m ²)	ESV (mL)	ESV index (mL/ m ²)	CO (L/min)	CI (L/min/ m ²)	SV (mL)	SV index (mL/ m ²)	EF (%)	Mass (g)	Mass index (g/m ²)	ED frame	ES frame
LV	116.79	77.57	37.87	25.15	5.05	3.36	78.92	52.42	67.58	77.52	51.49	29	11
RV	117.16	77.82	40.70	27.03	4.89	3.25	76.46	50.79	65.26	-	-	29	12

	Value
Classification	Normal
Confidence	0.95
Final Classification	Normal
BSA	1.51

GS2:

A warning shall be displayed stating CO, CI and other indexed volume metrics were not computed since heart rate, height and weight were not given.

	EDV (mL)	IEDV index (mL/m ²)	ESV (mL)	ESV index (mL/m ²)	CO (L/min)	CI (L/min/m ²)	SV (mL)	SV index (mL/m ²)	EF (%)	Mass (g)	Mass index (g/m ²)	ED frame	ES frame
LV	219.35	-	110.82	-	-	-	108.53	-	49.48	146.58	-	24	8
RV	203.11	-	91.67	-	-	-	111.44	-	54.87	-	-	24	9

	Value
Classification	Suspect
Confidence	0.69
Final Classification	Suspect
BSA	-

GS3:

The submission shall be disabled. A warning shall be displayed stating there are missing required fields.

3. The customer's IT Manager must send the validation report to AI4MedImaging's Field Support via email. The report must include:
 - A signed statement by the IT Manager confirming if the validation protocol was successful or if it failed.
 - Screenshots of the results obtained for the 3 golden samples.
4. AI4MedImaging's Field Support must confirm reception and sign the report. If the validation protocol is successful AI4MedImaging will provide the final user credentials to the customer. Otherwise, further support must be offered for problem resolution in articulation with the third-party plugin vendor.

3.4 User Training

After the setup is validated, the users will partake in individual or group training given by AI4MedImaging through the Microsoft Teams platform. The users must be trained before using AI4CMR.

Additional individual/group training or Demos can be requested and scheduled by contacting our Technical Support (Section 5).

3.5 Software overview

The AI4CMR operating sequence of events is summarized in Figure 2. The green-coloured boxes include the operations executed on the external DICOM Viewer plugin, to initiate AI4CMR processing (blue boxes).

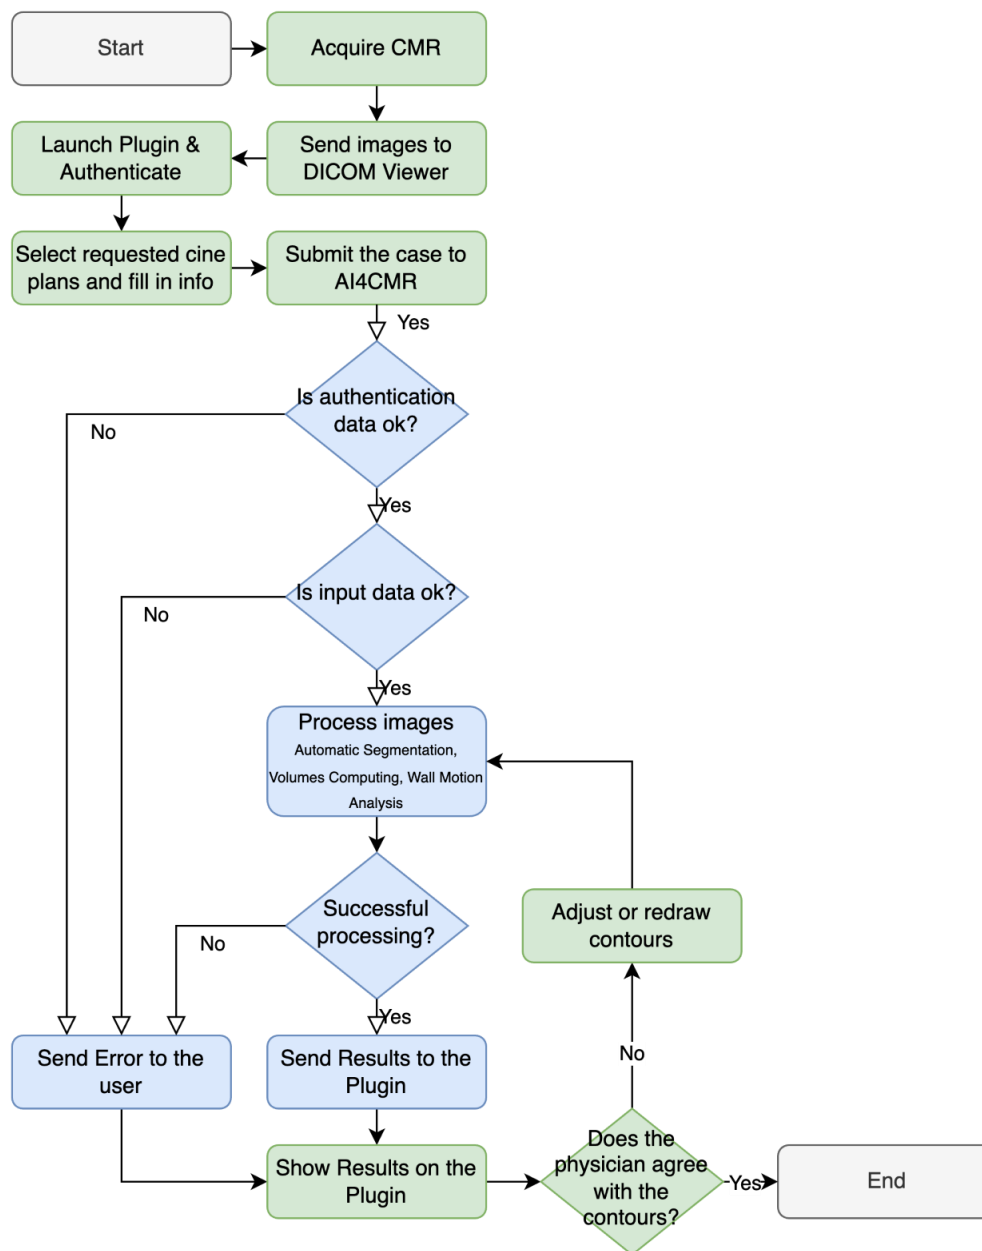


Figure 2. Flowchart of the operating sequence. Green steps are out of AI4CMR's control; blue steps are controlled by AI4CMR.

3.5.1 General operating steps

The general operating steps to use AI4CMR are summarized in the following table:

Operating step	System context
1. The Cardiac Magnetic Resonance is acquired according to standardized protocols	MRI Scanner
2. The images are sent to the third-party software	DICOM Viewer
3. The user launches the dedicated plugin on the third-party software and inserts the user credentials	Plugin
4. The user selects the correct cine sequence planes and other requested patient data	Plugin
5. The user submits the request form to the AI4CMR cloud service	Plugin
6. The request is subject to authentication	AI4CMR
7. The data on the request is checked for sanity and completion	AI4CMR
8. The patient data is processed by several AI-based image processing modules (myocardium automatic segmentation, ventricle volumes computation, wall motion analysis)	AI4CMR
9. The results and log messages (errors, warnings, ...) are collected and returned to the plugin via the communication API	AI4CMR
10. The user sees the output of AI4CMR on the dedicated plugin	Plugin
11. The user validates the outputs, or adjusts the contours on the dedicated plugin, prompting the ventricular volumes to be recomputed by AI4CMR.	Plugin/AI4CMR

A CMR case to be submitted to AI4CMR shall consist of:

1. Required:
 - DICOM cine SA with metadata:

- Image Patient Position;
 - Image Patient Orientation;
 - Pixel Spacing;
 - Slice Thickness;
 - Rows;
 - Columns.
 - Patient metadata:
 - Age (on acquisition date);
 - Sex.
2. Optional:
- DICOM cine 2ch, 3ch and 4ch (recommended);
 - Height, weight, heart rate.

The outputs of AI4CMR consist of:

- Left Ventricle endo and epicardium contours (coordinates)
- Right Ventricle endocardium contours (coordinates)
- Left Ventricle volumes-derived metrics:
 - EDV – End-Diastolic Volume [ml]
 - ESV – End-Systolic Volume [ml]
 - SV – Stroke Volume [ml]
 - EF – Ejection Fraction [%]
 - Mass – Myocardial Mass [g]
 - CO – Cardiac Output [L/min]
 - EDV/BSA – End-Diastole Volume/Body Surface Area [ml/m²]
 - ESV/BSA - End-Systole Volume/Body Surface Area [ml/m²]
 - SV/BSA – Systole Volume/Body Surface Area [ml/m²]
 - Mass/BSA – Myocardial Mass/Body Surface Area [g/m²]
 - CI – Cardiac Index [L/(min m²)]
 - BSA - Body Surface Area [m²]
- Right Ventricle volumes-derived metrics:
 - EDV – End-Diastolic Volume [ml]
 - ESV – End-Systolic Volume [ml]
 - SV – Stroke Volume [ml]
 - EF – Ejection Fraction [%]
 - CO – Cardiac Output [L/min]

- EDV/BSA – End-Diastole Volume/Body Surface Area [ml/m²]
- ESV/BSA - End-Systole Volume/Body Surface Area [ml/m²]
- SV/BSA – Systole Volume/Body Surface Area [ml/m²]
- CI – Cardiac Index [L/(min m²)]
- BSA - Body Surface Area [m²]
- Case classification:
 - Wall motion class – normal or suspect
 - Wall motion class confidence
 - Final class – normal or suspect

See Section 3.5.2 for details on outputs validation.

Notice:

1. The final case class takes both wall motion classification and ejection fraction value into account. A case is only deemed as normal if both criteria are in the normality range.
2. The “confidence” is a probability output (0-1) from the machine learning models used to classify each case. The closer the value is to 1, the greater the confidence in the attributed classification, taking the original training database¹ as a reference.

3.5.2 Summary of outputs validation

The studies conducted under the clinical evaluation phases showed high agreement between AI4CMR measurements and the human observers in a set of 146 patients:

- Correlation (ICC) in the measurement of LV EDV is 0.99, LV ESV is 0.99, LV SV is 0.83, LV EF is 0.96 and Mass is 0.96. The other volume metrics are arithmetically derived from the previous.
- The accuracy and precision of the measurement of the volume are given by the bias (mean difference) and the standard deviation:

	LV EDV (ml)	LV ESV (ml)	LV SV (ml)	Mass (g)	LV EF (%)
AI4CMR vs consensus (*)	1.81±17.61	- 6.84±17.65	8.36±17.25	3.19±17.37	3.86±5.80

¹ Training database - Neural networks and other artificial intelligence programs require an initial set of data, called training data, to act as a baseline for further application and utilization. AI4CMR has been trained, validated and tested on a split database of around 1000 patients, labelled by experts.

- Correlation (ICC) in the measurement of RV EDV is 0.97, RV ESV is 0.94, RV SV is 0.82 and RV EF is 0.80. The other volume metrics are arithmetically derived from the previous.
- The accuracy and precision on the measurement of the volume are given by the bias (mean difference) and the standard deviation:

	RV EDV (ml)	RV ESV (ml)	RV SV (ml)	RV EF (%)
AI4CMR vs rater1 (*)	1.25±15.99	-13.26±14.63	14.24±15.53	8.34±7.34

(*) The consensus between 2 raters (experts) was obtained by averaging each measurement. The measurements were obtained through a certified software, which computes the volumes based on the raters' manual segmentations.

- For case classification, the sensitivity is 100%, the negative predictive value is 100%, the accuracy is 76.7%, the positive predictive value is 70% and the specificity is 50%.

No uncertainty/error information is shown in the software together with the LV measurements.

3.5.3 Plugin

AI4CMR is intended to be integrated with a third party DICOM Viewer. The integration is established via a communication protocol implemented by a Plugin. AI4CMR does not have a User Interface. The end-user will interact with AI4CMR via the Plugin's interface.

The Plugin User Manual or Guide, which accompanies the current manual, describes in more detail the features and steps necessary to interact with the AI4CMR service. The Plugin consists of a user interface to help the User create the request form.

Different viewers can have different user experiences, but the main idea should be the same.

For clarification purposes, this section provides merely indicative (not binding) examples of what the user experience may be like with a third-party Plugin for AI4CMR.

Login

The first step to use the AI4CMR is to successfully authenticate with the service. To do that, there are two options:

- The User shall provide a username and password through the user interface

- The plugin loads credentials/licensing information securely saved in or transmitted by the User's system.

Figure 3. Example of a plugin login window.

Input Data Selection

The input data selection can be done in two ways:

- Manually by the User through the user interface. This option may or may not include automatic prefilling.
- Automatically by the plugin taking advantage of the standard DICOM tags.

Form filling

Figure 4 shows an example of an interface for the User to fill in the necessary information. The automation of this step is advised and should allow the edition of the patient metadata (age, sex, heart rate, height, and weight) and the cine slices (cine_sa (SA), cine_2ch (LA 2ch), cine_3ch (LA 3ch), and cine_4ch (LA 4ch)).

AI4CMR's performance has been validated for a range of image characteristics, as shown in the tables² below:

Ranges	Number of Pixel Rows	Number of Pixel Columns	Image Size Values	Slice Thickness Values
Error	$]-\infty, 140[$	$]-\infty, 140[$	$]-\infty, 26957[$	$]-\infty, 7.2[$
Warning	$[140, 156[$	$[140, 156[$	$[26957, 29952[$	$[7.2, 8[$
Acceptance	$[156, 320]$	$[156, 320]$	$[29952, 102400]$	8
Warning	$]320, 352]$	$]320, 352]$	$]102400, 123904]$	$]8, 8.8]$
Error	$]352, +\infty[$	$]352, +\infty[$	$]123904, +\infty[$	$]8.8, +\infty[$

² The values are the result of a study conducted based on a significative sample of CMR cases.

Ranges	Pixel Spacing Values	Number of Slices	Slice Spacing Values	Pixel Intensity Values
Error	$]-\infty, 0.8389[$	$]-\infty, 8[$	$]-\infty, 7.2[$	$]-\infty, 28.0069[$
Warning	$[0.8389, 0.9322[$	$[8, 9[$	$[7.2, 8[$	$[28.0069, 31.1188[$
Acceptance	$[0.9322, 1.7709]$	$[9, 16]$	$[8, 10]$	$[31.1188, 273.8040]$
Warning	$]1.7709, 1.9479]$	$]16, 19]$	$]10, 11.2]$	$]273.8040, 355.1480]$
Error	$]1.9479, +\infty[$	$]19, +\infty[$	$]11.2, +\infty[$	$]355.1480, +\infty[$

Cases with image characteristics that are outside the boundaries of the verified performance of the algorithms will be rejected.

Patient metadata shall be filled in by the User if the Plugin does not automatically fill it based on the DICOM information:

- Mandatory:
 - Patient ID
 - Age
 - Sex
- Optional:
 - Heart rate (if not sent to AI4CMR: CO and CI will not be computed)
 - Height (if not sent to AI4CMR: no BSA nor indexed metrics (EDV/BSA, ESV/BSA, SV/BSA, Mass/BSA, CI) will be computed)
 - Weight (if not sent to AI4CMR: no BSA nor indexed metrics (EDV/BSA, ESV/BSA, SV/BSA, Mass/BSA, CI) will be computed)

Figure 4. Example of a plugin form filling window.

Results presentation

After successful processing, the plugin presents the results. The results presentation includes someway to show contours and someway to show numerical values and text. In the case of failure, an error message shall be outputted instead of the results.

One example of a possible user interface for results reporting is presented in the bottom half of Figure 5 (LV report) and Figure 6 (RV Report).

The screenshot displays the AI4MedImaging Plugin v1.3 interface. At the top, there is a 'connection status' button, the AI4MedImaging logo, and a 'Reset' button. Below this is the 'Input patient data' section, which includes input fields for patient ID, age, sex, heart rate, height, and weight. There are also four image placeholders labeled SA, LA 2ch, LA 3ch, and LA 4ch. A 'submit' button is located below these inputs, followed by a blue progress bar. Below the progress bar are two tabs: 'LV Report' (selected) and 'RV Report'. The 'LV Report' section contains a 'Wall Motion' section with a 'Classification:' field and a 'Confidence:' field. Below this is a 'Volumes' section with a table of cardiac parameters. At the bottom, there is a 'Feedback' button, a 'Final classification:' field, and a question mark icon.

Volumes		
End Diastole Volume:	End Diastole Volume Index:	Cardiac Index:
End Systole Volume:	End Systole Volume Index:	End Diastole Frame:
Stroke Volume:	Stroke Volume Index:	End Systole Frame:
Myocardium Mass:	Myocardium Mass Index:	Body Surface Area:
Ejection Fraction:	Cardiac Output:	

Figure 5. Example of a plugin form filling and results in the presentation window – LV Report.

The screenshot shows a web application window titled "Plugin" with a version indicator "v1.3". At the top left is a "connection status" button, followed by the "AI4MedImaging" logo, and a "Reset" button at the top right.

Below the header is a section titled "Input patient data" containing six input fields arranged in two rows: "patient ID:", "age:", "sex:" in the first row, and "heart rate:", "height:", "weight:" in the second row. Below these fields is a large gray square placeholder labeled "SA".

At the bottom of the input section is a "submit" button and a blue progress bar.

Below the submit button are two tabs: "LV Report" and "RV Report". The "RV Report" tab is selected.

Under the "RV Report" tab is a table titled "Volumes":

Volumes		
End Diastole Volume:	End Diastole Volume Index:	Cardiac Index:
End Systole Volume:	End Systole Volume Index:	End Diastole Frame:
Stroke Volume:	Stroke Volume Index:	End Systole Frame:
Ejection Fraction:	Cardiac Output:	Body Surface Area:

At the bottom left is a "Feedback" button, and at the bottom right is a circular help icon with a question mark.

Figure 6. Example of a plugin form filling and results in the presentation window – RV Report.

Additional fields

Connection status

This field is used to indicate that the AI4CMR service is available.

If not, the User should be able to force a connection status update. Either by clicking on the status or using any other way. The connection check endpoint of CORE should be used here to test the connection.



Figure 7. Connection status example.

Reset button

The reset button is used to clean all the info from the current request and make it easier for the user to start a new request without cleaning each field individually.

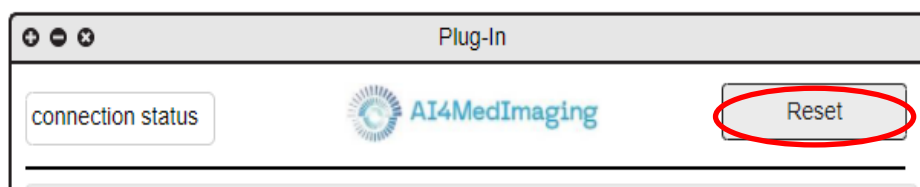


Figure 8. Reset button example.

Info button

This button presents information regarding the plugin and AI4CMR service, such as email, certifications, versions, device labelling and so on.

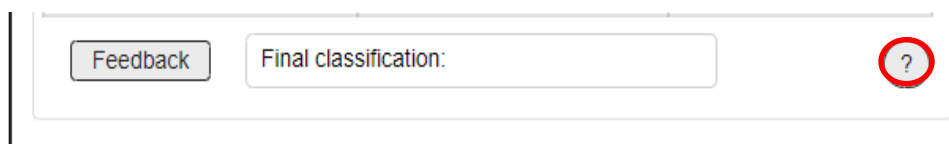


Figure 9. Info button example.

Confidence disclaimer

This button presents information to clarify the wall motion classification results. When clicked, the button should display the disclaimer text.

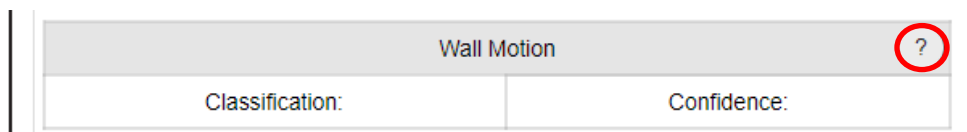


Figure 10. Confidence disclaimer button example.

Feedback button

This button can be used to redirect the User to a feedback webpage, email software, present a mobile number or any other communication way that might fit the task of providing feedback or requesting assistance. The plugin team can also include (or prefill) the message to be sent so that possible problems are easier to track.

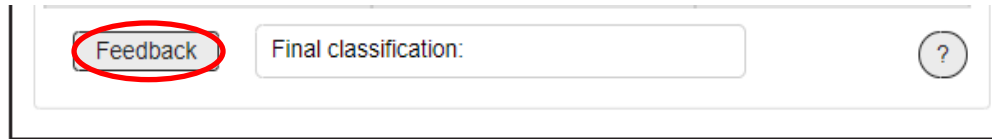


Figure 11. Feedback button example.

4. User account handling


The AI4CMR provides a user account handling page, that allows each user to change their personal information and credentials. To access this functionality, the user should use the following link via the Google Chrome browser (minimum recommended version: 97) or the Safari browser (minimum recommended version: 14.1):

- <https://auth.ai4medimaging.com/auth/realms/srrealm/account>

4.1 Authentication

To access the account, the user should provide the assigned username or email and password.

Note: the authentication/login window depends on the third-party plugin integration.

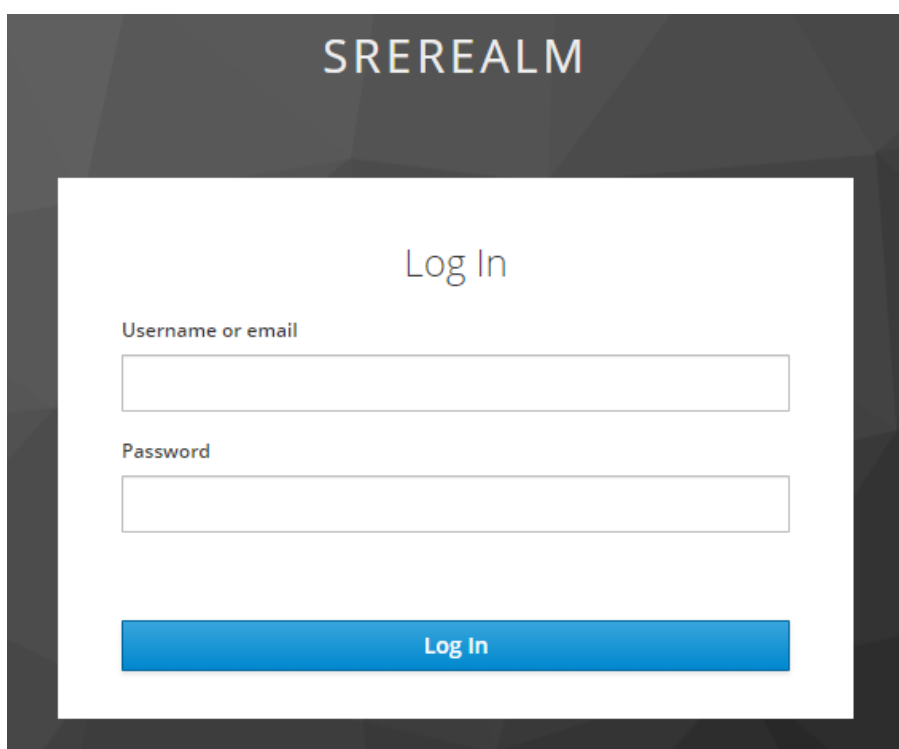


The image shows a login interface for 'SRERealm'. At the top, the word 'SRERealm' is displayed in a large, white, sans-serif font against a dark grey background. Below this, there is a white rectangular area containing the login form. The form has the text 'Log In' centered at the top in a grey font. Underneath, there are two input fields: the first is labeled 'Username or email' and the second is labeled 'Password'. Both labels are in a small, grey font. Below the password field is a blue button with the text 'Log In' in white.

Figure 12. User account login page.

After successful authentication the user handling page will be presented, Figure 13.

4.2 User information handling

After logging in, on the separator “Account” the user can change the email, first name and last name by filling the respective field and clicking on “Save”. If these values already exist, they will be presented in the respective field.

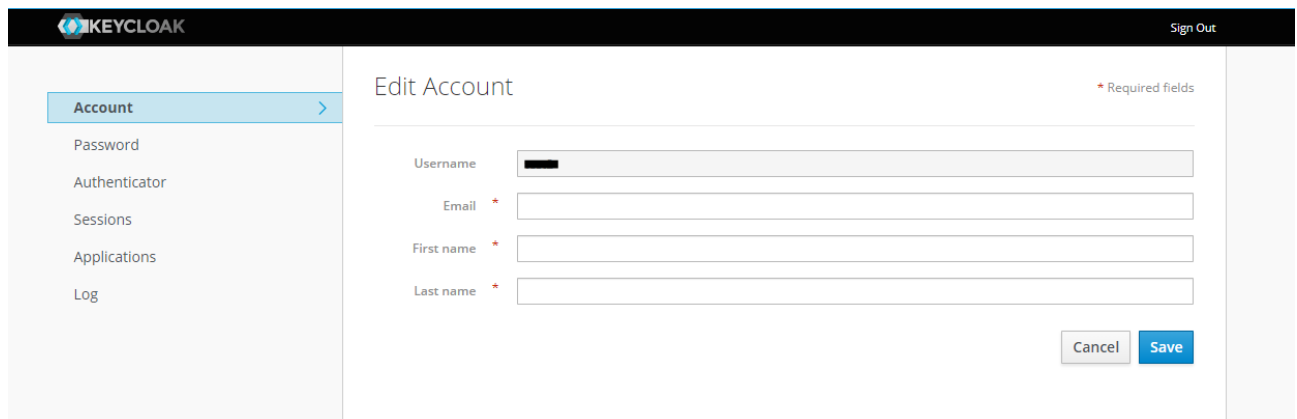


The screenshot shows the Keycloak 'Edit Account' interface. On the left, a sidebar contains links for 'Account', 'Password', 'Authenticator', 'Sessions', 'Applications', and 'Log'. The 'Account' link is highlighted. The main content area is titled 'Edit Account' and includes a red asterisk indicating required fields. It contains four input fields: 'Username' (with a masked value), 'Email', 'First name', and 'Last name'. A 'Sign Out' link is located in the top right corner. At the bottom right, there are 'Cancel' and 'Save' buttons.

Figure 13. User account personal information edit page.

4.3 Password handling

To change the password, the user should log in first and change to the “Password” separator, provide the current password on the “Password” field and the new password on the “New Password” and “Confirmation” fields. After clicking on “Save” the password will be updated.

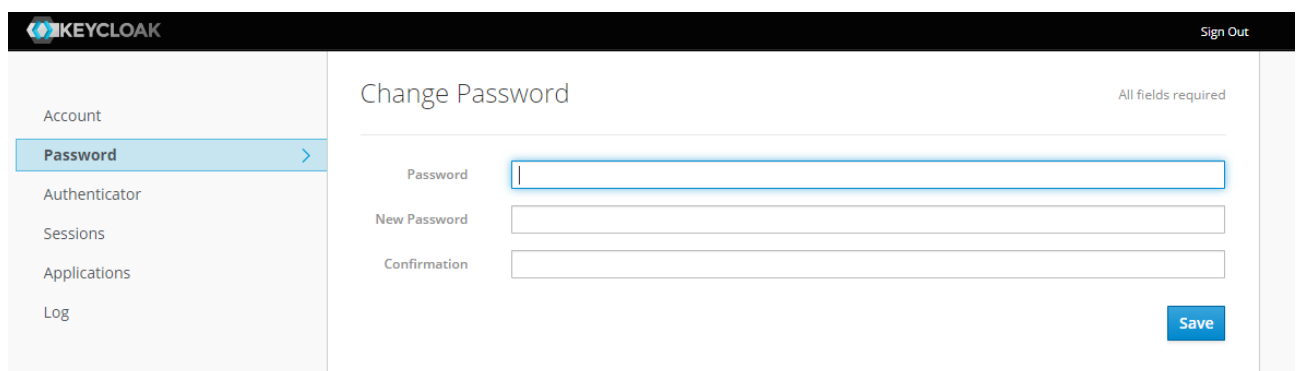

The screenshot shows the Keycloak 'Change Password' interface. On the left, a sidebar contains links for 'Account', 'Password', 'Authenticator', 'Sessions', 'Applications', and 'Log'. The 'Password' link is highlighted. The main content area is titled 'Change Password' and includes a note 'All fields required'. It contains three input fields: 'Password', 'New Password', and 'Confirmation'. A 'Sign Out' link is located in the top right corner. At the bottom right, there is a 'Save' button.

Figure 14. User account password edit page.

In case of password loss or account compromised, the IT Manager of the User's Institution should contact the AI4MedImaging's Technical Support (see section 5 for details).

4.4 Open sessions

The user has the option to monitor all open sessions associated with his account. That information is accessible in the “Sessions” separator. If any of the sessions open is considered suspect, the user has the option to close it using the “Log out all sessions” button.

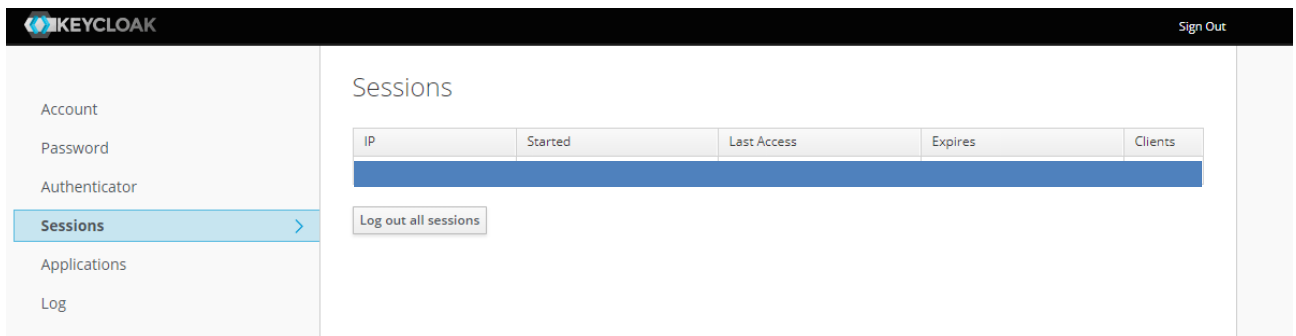


Figure 15. User account open sessions page.

4.5 Logging info

In addition to the open sessions, the user has the option to see all logging events that happen using his account. This information can be accessed on the “Log” separator.

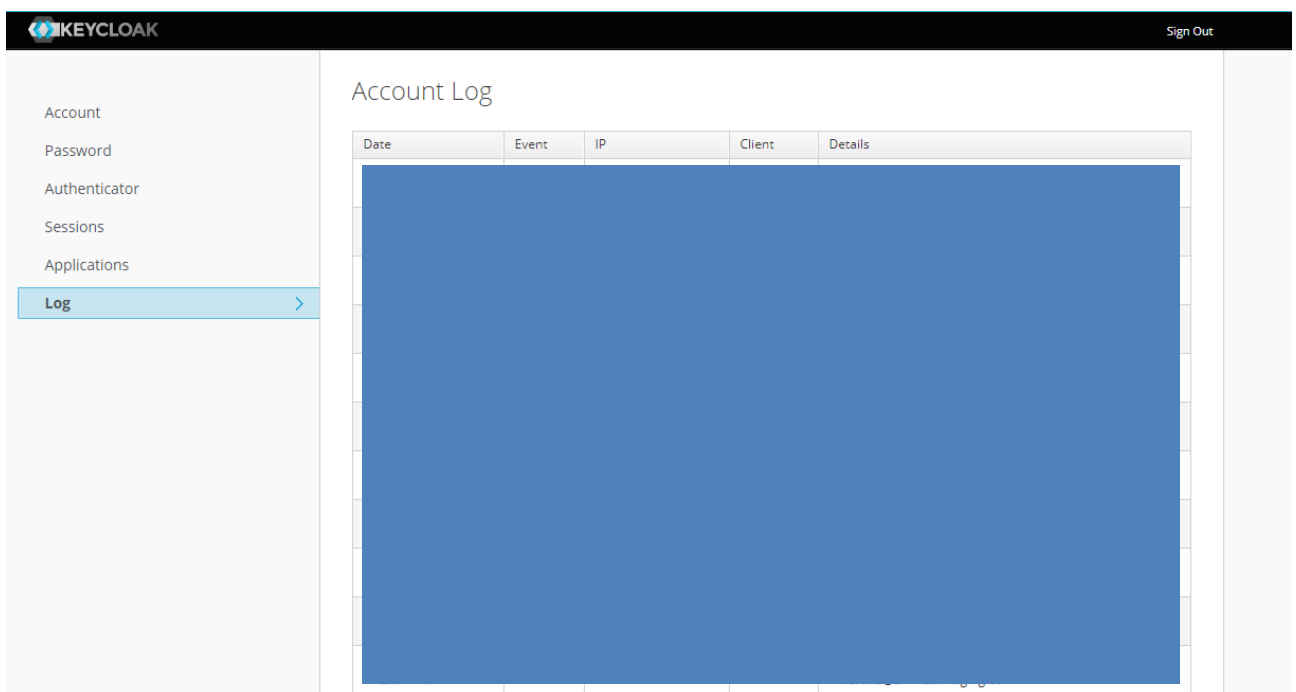


Figure 16. User account access log page.

5. Technical Support

For technical questions, to report a problem, or to request individual/group training or demos, please contact our team by e-mail or website:

AI4MedImaging Medical Solutions S.A.

Rua do Parque Poente, Lote 35
4705-002 Sequeira, Braga
Portugal

Website: <https://ai4medimaging.com/>

E-mail: support@ai4medimaging.com